


PERIODIC CALIBRATION

Kathy Stolper Visual Estimates of Cementation Exponent Archie "m" vs Measured Core Values

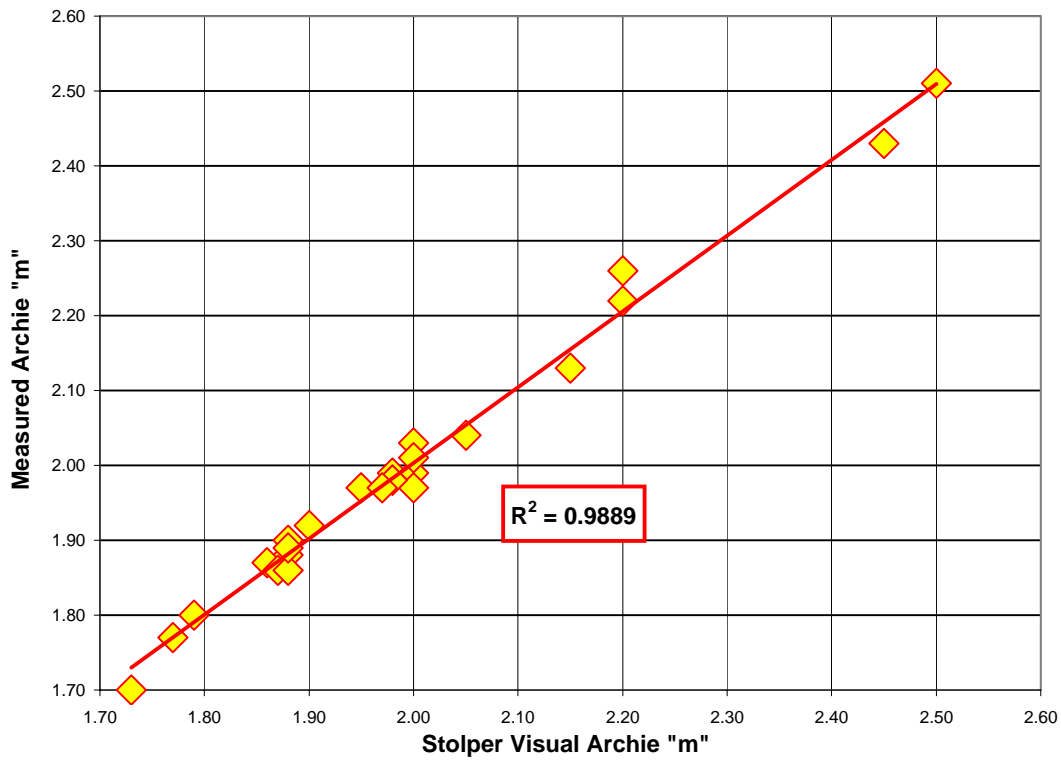

Spl Ref #	Stolper Visual Est.m	Measured m
1	1.80	1.78
2	1.92	1.93
3	2.15	2.15
4	1.80	1.79
5	1.96	1.96
6	1.84	1.83
7	1.73	1.72
8	1.96	1.96
9	2.05	2.08
10	1.92	1.91
11	2.05	2.09
12	1.80	1.71
13	1.90	1.90
14	1.92	1.92
15	2.10	2.06
16	1.86	1.86
17	1.77	1.75
18	1.90	1.88
19	2.00	2.00
20	1.80	1.73
21	1.93	1.93
22	1.87	1.87
23	1.80	1.81
24	2.00	2.07
25	1.96	1.96

Spl Ref #	Stolper Visual Est.m	Measured m
26	1.88	1.88
27	1.79	1.80
28	2.05	2.04
29	1.88	1.90
30	1.98	1.99
31	2.00	1.99
32	1.98	1.98
33	2.20	2.22
34	2.00	2.03
35	2.00	1.97
36	1.98	1.98
37	1.86	1.87
38	1.77	1.77
39	1.95	1.97
40	1.97	1.97
41	2.20	2.26
42	1.73	1.70
43	1.87	1.86
44	1.88	1.86
45	1.88	1.89
46	1.90	1.92
47	2.00	2.01
48	2.45	2.43
49	2.15	2.13
50	2.50	2.51